

Importance of Fluoroquinolone Determination

Antibiotic residues in foods pose a serious threat to public health. This is especially true of the Fluoroquinolones, a class of broad-spectrum antibiotics whose use in both humans and animals is restricted in many countries due to the quantity and severity of potential adverse effects. These effects occur during or even long after use and include central nervous system toxicity, peripheral neuropathy, blood disorders, and brain, liver, endocrine, musculoskeletal and gastrointestinal dysfunction. The FDA has recommended black box warnings for all Fluoroquinolone antibiotics due to the risk of tendonitis and tendon rupture. Several Fluoroquinolones have been removed from clinical use due to human fatalities. Side effects are most severe among the elderly and in children. Fluoroquinolones are not approved or are severely restricted for use in children in many countries and should not be taken by women who are pregnant or breastfeeding. Although banned for use in all food animals in Australia, as well as poultry and fish in the United States (due to the sharp increase in Ciprofloxacin resistant *Campylobacter* infections transmitted to humans), Fluoroquinolones are routinely used for veterinary treatment in a variety of food animals in many countries, including China, most countries in the EU and Japan. Fluoroquinolones are administered to treat infections and are also given prophylactically in feed or drinking water. The monitoring of water sources and food products such as meat and milk for antibiotic residues is necessary to ascertain that these compounds are not misused and do not present a danger to human or animal health.


The Abraxis Fluoroquinolones ELISA allows the determination of 41 samples in duplicate determination. Only a few grams or milliliters of sample are required. The test can be performed in less than 2 hours.

Performance Data

Test sensitivity: The limit of detection for Fluoroquinolones, calculated as 90% B/Bind, is approximately 0.016 ng/mL.

Standard Curve: The concentration of residue necessary to cause 50% inhibition (50% B/B₀) is approximately 0.19 ng/mL. Determinations closer to the middle of the calibration range of the test yield the most accurate results.

These values are used for demonstration purposes only; do not use these values for your determinations:

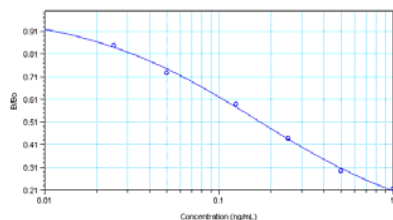

Test reproducibility: Coefficients of variation (CVs) for standards: <10%; CVs for samples: <15%.

Selectivity/
Cross-reactivity: This ELISA recognizes various Fluoroquinolones with varying degrees:

Enrofloxacin	100%
Danofloxacin	100%
Ciprofloxacin	66%
Fleroxacin	25%
Enoxacin	17%
Pefloxacin	12%
Ofloxacin	11%
Norfloxacin	7%
Marbofloxacin	6%
Levofloxacin	5%
Sarafloxacin	<1%
Oxolinic Acid	<1%

Samples: To eliminate matrix effects in fish or shrimp samples, sample clean-up is required. See Preparation of Samples, section H.

General Limited Warranty: Abraxis LLC warrants the products manufactured by the Company against defects and workmanship when used in accordance with the applicable instructions for a period not to extend beyond the product's printed expiration date. **Abraxis makes no other warranty, expressed or implied. There is no warranty of merchantability or fitness for a particular purpose.**

For ordering or technical assistance contact: Abraxis LLC
54 Steamwhistle Drive
Warminster, PA 18974
Tel.: (215) 357-3911
Fax: (215) 357-5232
Email: info@abraxiskits.com
WEB: www.abraxiskits.com

R030110

Fluoroquinolones ELISA, Microtiter Plate

Enzyme-Linked Immunosorbent Assay for the Determination
of Fluoroquinolones in Contaminated Samples

Product No. 52250BA



1. General Description

The Fluoroquinolones ELISA is an immunoassay for the detection of Fluoroquinolones. This test is suitable for the quantitative and/or qualitative detection of Fluoroquinolones in contaminated samples including water, fish and shellfish (please refer to the appropriate technical bulletins for additional extraction/dilution procedures). Samples requiring regulatory action should be confirmed by HPLC, GC/MS, or other conventional methods.

2. Safety Instructions

The standard solutions in this test kit contain small amounts of Enrofloxacin. In addition, the substrate solution contains tetramethylbenzidine and the stop solution contains diluted sulfuric acid. Avoid contact of stopping solution with skin and mucous membranes. If these reagents come in contact with the skin, wash with water.

3. Storage and Stability

The Fluoroquinolones ELISA Kit should be stored in the refrigerator (4–8°C). The solutions must be allowed to reach room temperature (20–25°C) before use. Reagents may be used until the expiration date on the box. The conjugate is supplied in lyophilized form (3 vials). Before each assay, the required volume of lyophilized conjugate must be reconstituted with the appropriate diluent (see Test Preparation section). Reconstitute only the amount needed for the samples to be run, as the reconstituted solution will only remain viable for one week (store refrigerated).

4. Test Principle

The test is a direct competitive ELISA based on the recognition of Fluoroquinolones by specific antibodies. Fluoroquinolones, when present in a sample, and a Fluoroquinolone-enzyme conjugate compete for the binding sites of rabbit anti-Fluoroquinolone antibodies in solution. The Fluoroquinolone antibodies are then bound by a second antibody (goat anti-rabbit) immobilized on the microtiter plate. After a washing step and addition of the substrate solution, a color signal is produced. The intensity of the blue color is inversely proportional to the concentration of Fluoroquinolones present in the sample. The color reaction is stopped after a specified time and the color is evaluated using a microplate ELISA photometer. The concentrations of the samples are determined by interpolation using the standard curve constructed with each run.

5. Limitations of the Fluoroquinolones ELISA, Possible Test Interference

Numerous organic and inorganic compounds commonly found in samples have been tested and found not to interfere with this test. However, due to the high variability of compounds that might be found in samples, test interferences caused by matrix effects can not be completely excluded. Mistakes in handling the test can also cause errors. Possible sources for such errors can be:

Inadequate storage conditions of the test kit, incorrect pipetting sequence or inaccurate volumes of the reagents, too long or too short incubation times during the immune and/or substrate reaction, extreme temperatures during the test performance (lower than 10°C or higher than 30°C).

The Abraxis Fluoroquinolones ELISA kit provides screening results. As with any analytical technique (GC, HPLC, etc.), samples requiring regulatory action should be confirmed by an alternative method.

Working Instructions

A. Materials Provided

1. Microtiter plate coated with a second antibody (goat anti-rabbit).
2. Fluoroquinolone Standards (7): 0, 0.025, 0.05, 0.125, 0.25, 0.5, and 1.0 ng/mL.
3. Fluoroquinolone-HRP Conjugate, 3 vials (lyophilized). 3 mL/vial after reconstitution.
4. Conjugate Diluent, 12 mL.
5. Rabbit Anti-Fluoroquinolone Antibody Solution, 6 mL.
6. Sample Diluent, 25 mL. Use to dilute samples.
7. Wash Solution (5X) Concentrate, 100 mL.
8. Color (Substrate) Solution (TMB), 12 mL.
9. Stop Solution, 12 mL.

B. Test Preparation

Micro-pipetting equipment and pipette tips for pipetting the standards and the samples are necessary. We recommend using a multi-channel pipette or a stepping pipette for adding the conjugate, antibody, substrate and stop solutions in order to equalize the incubation periods of the solutions on the entire microtiter plate. Please use only the reagents and standards from one package lot in one test, as they have been adjusted in combination.

1. Adjust the microtiter plate and the reagents to room temperature before use.
2. Remove the number of microtiter plate strips required from the foil bag. The remaining strips are stored in the foil bag and zip-locked closed. Store the remaining kit in the refrigerator (4-8°C).
3. The standard solutions, antibody, substrate and stop solutions are ready to use and do not require any further dilutions.
4. The conjugate provided is lyophilized (3 vials). Before each assay, calculate the volume of conjugate needed (when reconstituted, each vial will provide enough conjugate for approximately 50 wells). Reconstitute only the amount necessary for the samples to be analyzed. Once reconstituted, the conjugate solution will only remain viable for 1 week (store refrigerated). If additional samples are to be analyzed greater than one week from reconstitution, a new vial of conjugate must be prepared. To reconstitute, add 3 mL of Conjugate Diluent to each vial of Conjugate required and vortex thoroughly.
5. Dilute the wash buffer concentrate at a ratio of 1:5. If using the entire bottle (100 mL), add to 400 mL of deionized or distilled water.
6. The stop solution should be handled with care as it contains diluted H₂SO₄.

C. Assay Procedure

1. Add 50 µL of the standard solutions and samples or sample extracts into the wells of the test strips according to the working scheme given. We recommend using duplicates or triplicates.
2. Add 50 µL of reconstituted enzyme conjugate solution to the individual wells successively using a multi-channel pipette or a stepping pipette.
3. Add 50 µL of antibody solution to the individual wells successively using a multi-channel pipette or a stepping pipette. Cover the wells with parafilm or tape and mix the contents by moving the strip holder in a circular motion on the benchtop for 30 seconds. Be careful not to spill contents.
4. Incubate the strips for 60 minutes at room temperature.
5. After incubation, remove the covering and vigorously shake the contents of these wells into a sink. Wash the strips three times using the 1X washing buffer solution. Use at least a volume of 250 µL of washing buffer for each well and each washing step. Remaining buffer in the wells should be removed by patting the plate dry on a stack of paper towels.
6. Add 100 µL of color (substrate) solution to the wells. Cover the wells with parafilm or tape and mix the contents by moving the strip holder in a circular motion on the benchtop for 30 seconds. Incubate the strips for 20-30 minutes at room temperature. Protect the strips from direct sunlight.
7. Add 100 µL of stop solution to the wells in the same sequence as for the substrate solution.
8. Read the absorbance at 450 nm using a microplate ELISA photometer within 15 minutes after the addition of the stopping solution.

D. Evaluation

The evaluation of the ELISA can be performed using commercial ELISA evaluation programs (4-Parameter (preferred) or Logit/Log). For manual evaluation, calculate the mean absorbance value for each of the standards. Calculate the %B/B₀ for each standard by dividing the mean absorbance value for each standard by the Zero Standard (Standard 0) mean absorbance. Construct a standard curve by plotting the %B/B₀ for each standard on the vertical linear (y) axis versus the corresponding Fluoroquinolones concentration on the horizontal logarithmic (x) axis on graph paper. %B/B₀ for samples will then yield levels in ppb of Fluoroquinolones by interpolation using the standard curve. Samples showing a higher concentration than Standard 6 (1.0 ng/mL) must be diluted further to obtain accurate results.

E. Additional Materials (not included with the test kit)

1. Micro-pipettes with disposable plastic tips (10-200 and 200-1000 µL)
2. Multi-channel pipette (10-250 µL) or stepper pipette with plastic tips (10-250 µL)
3. Microtiter plate reader (wave length 450 nm)
4. Timer
5. Tape or Parafilm

F. Working Scheme

The microtiter plate consists of 12 strips of 8 wells, which can be used individually for the test. The standards must be run with each test. Never use the values of standards which have been determined in a test performed previously.

Std 0-Std 6: Standards

0; 0.025; 0.05; 0.125; 0.25; 0.5; 1.0 ppb

Samp1, Samp2, etc.: Samples

	1	2	3	4	5	6	7	8	9	10	11	12
A	Std 0	Std 4	Samp2									
B	Std 0	Std 4	Samp2									
C	Std 1	Std 5	etc.									
D	Std 1	Std 5	etc.									
E	Std 2	Std 6										
F	Std 2	Std 6										
G	Std 3	Samp1										
H	Std 3	Samp1										

G. Preparation of Samples

Water

Water samples should be collected in glass vessels with Teflon lined caps. Prior to analysis, each sample must be diluted with methanol (HPLC grade) to a 10% v/v final concentration of methanol (i.e. 100 µL of methanol into 900 µL of sample).

The Fluoroquinolones concentration in the sample is determined by multiplying the ELISA results of the prepared sample by 1.1. Highly contaminated samples (those outside of the calibration range of the assay) must be diluted with sample diluent and re-analyzed.

Fish/Shrimp

1. Weigh 1g of homogenized fish or de-shelled shrimp (should have a paste-like consistency) into a 10 mL or larger glass vial with a Teflon lined cap.
2. Add 3 mL of 80% Methanol to vial. Vortex thoroughly. Mix using an overhead tube rotator for 20 minutes.
3. Centrifuge vial for 10 minutes at 2000 g. Pipette 2 mL of the supernatant (top layer) into a clean vial.
4. Centrifuge extract for 10 minutes at 2000 g (centrifuging the 2 mL of supernatant separately removes a greater amount of matrix interference from the extract to be analyzed).
5. Pipette 1 mL of the supernatant (top layer) into a clean vial.
6. Add 100 µL of the final extract to 900 µL of Sample Diluent and vortex thoroughly. This will then be analyzed as sample (Assay Procedure, step 1).

The Fluoroquinolones concentration in the sample is determined by multiplying the ELISA results of the diluted extract by a factor of 40 (range of detection of the assay will be 1.0 – 40.0 ng/mL). Highly contaminated samples (those outside of the calibration range of the assay) must be diluted and re-analyzed. Samples of shrimp and fish were spiked with Enrofloxacin and extracted using the above procedure. Recoveries were 85-103%.

Honey


1. Weigh 1 g of honey in a glass vial and add 1 mL of sample diluent (10% MeOH in 1X PBS, pH 7.0-7.4)
2. Vortex vigorously for 2 minutes
3. Dilute samples 1:12.5 as follows: 50 µL of sample (step 2) and 575 µL of sample diluent. This will then be analyzed as sample (Assay Procedure, step 1). The Fluoroquinolones concentration in the sample is determined by multiplying the ELISA results of the prepared sample by 25.

Samples of honey were spiked with Enrofloxacin and extracted using the above procedure. Recoveries were 100-103%.

Fluoroquinolones Plate, Detailed ELISA Procedure


1. Addition of Calibrators, Samples

Add 50 μ L of calibrators or sample extracts into the wells of the test strips according to the working scheme given. We recommend using duplicates or triplicates.

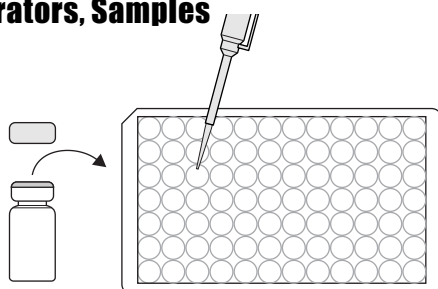


2. Addition of Enzyme Conjugate

Add 50 μ L of the Enzyme Conjugate to the individual wells successively using a multi-channel pipette.

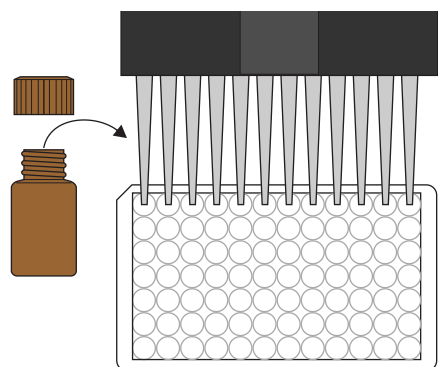


3. Addition of Antibody Solution

Add 50 μ L of the Antibody solution to the individual wells successively using a multi-channel pipette or a stepping pipette. Cover the wells with parafilm or tape and mix the contents by moving the strip holder in a rapid circular motion on the benchtop. Be careful not to spill contents. Incubate the strips for 30 min at room temperature.

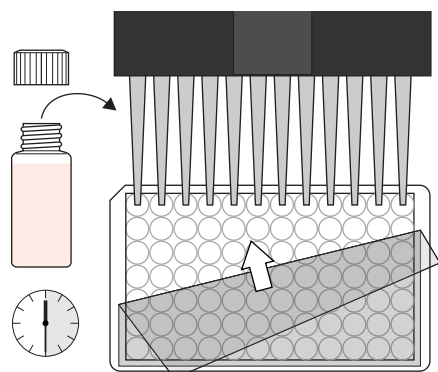


4. Washing of Plates

After incubation, remove the covering and vigorously shake the contents of the wells into a sink. Wash the strips three times with a multi-channel pipette or wash bottle using the diluted 1X washing buffer solution. Please use at least a volume of 250 μ L of washing buffer for each well and each washing step. Remaining buffer in the wells should be removed by patting the plate dry on a stack of paper towels. Repeat steps an additional three times.

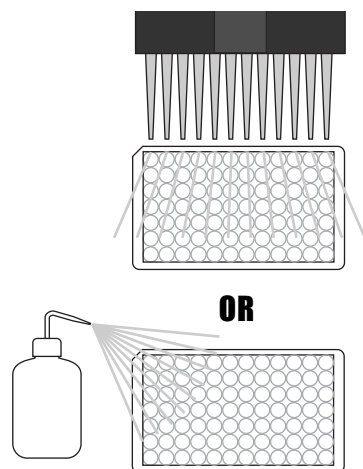


5. Addition of Substrate/Color Solution

Add 100 μ L of substrate/color solution to the individual wells successively using a multi-channel pipette or a stepping pipette. Cover the wells with parafilm or tape and mix the contents by moving the strip holder in a rapid circular motion on the benchtop. Be careful not to spill contents. Incubate the strips for 30 min at room temperature.

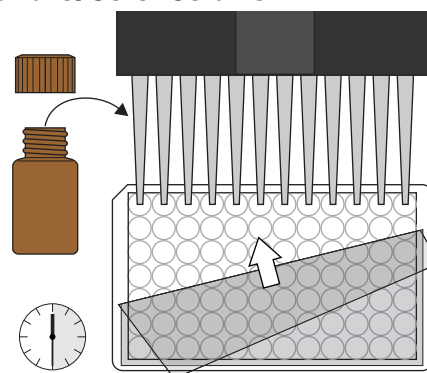


6. Addition of Stopping Solution

Add 100 μ L of stop solution to the wells in the same sequence as for the substrate solution using a multi-channel pipette or a stepping pipette.

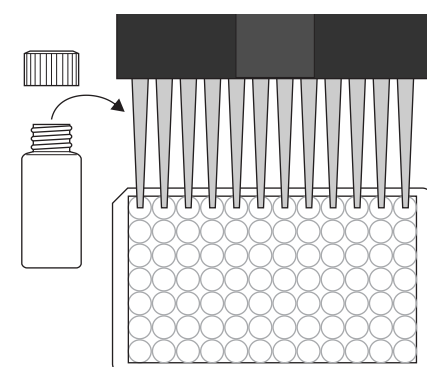

7. Measurement of Color

Read the absorbance at 450 nm using a microplate ELISA reader. Calculate results.

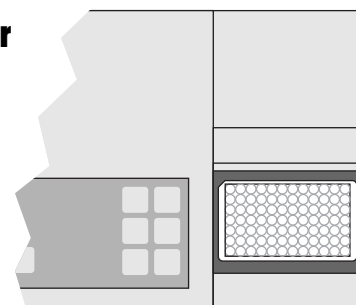


For Ordering or Technical Assistance Contact:
ABRAXIS, LLC
54 Steamwhistle Drive, Warminster, PA 18974
Phone: 215-357-3911 Fax: 215-357-5232
www.abraxiskits.com

Fluoroquinolones Plate, Concise ELISA Procedure


1. Addition of Standards, Samples

Add 50 μ L of calibrators or samples.

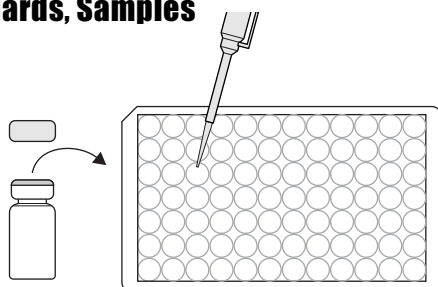


2. Addition of Enzyme Conjugate

Add 50 μ L of the enzyme conjugate.

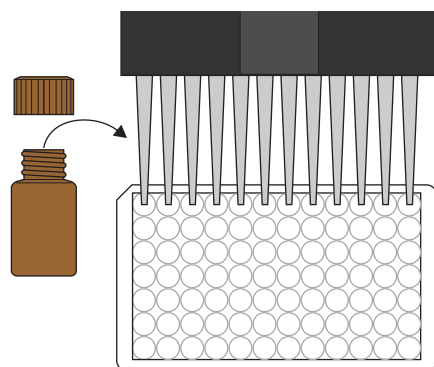


3. Addition of Antibody Solution

Add 50 μ L of Antibody solution. Cover and mix for 30 seconds by rotating on benchtop. Incubate for 30 minutes at room temperature.

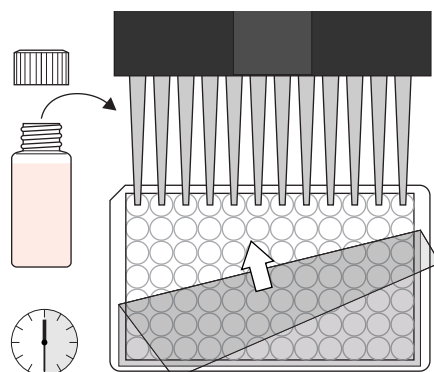


4. Washing of Plates

Wash the plates four times with 250 μ L of diluted 1X washing buffer.

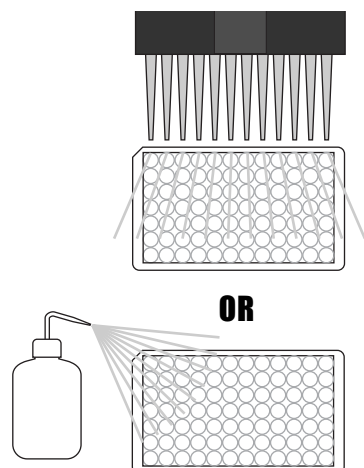


5. Addition of Substrate/Color Solution

Add 100 μ L of substrate/color solution. Incubate 30 minutes at room temperature and away from direct sunlight.

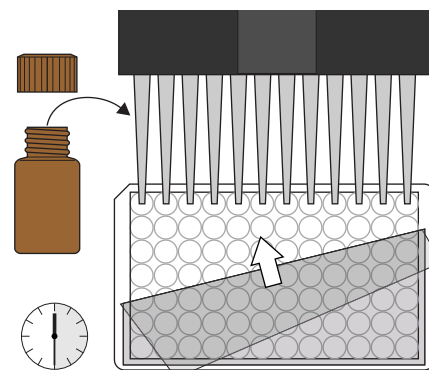


6. Addition of Stopping Solution

Add 100 μ L of stop solution.

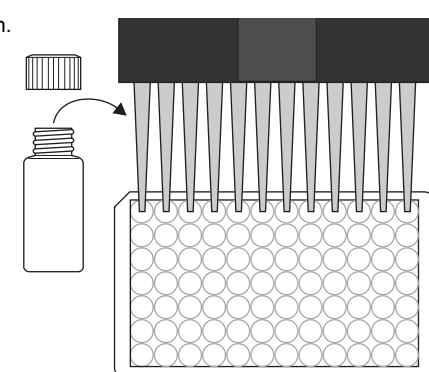

7. Measurement of Color

Measure color at 450 nm. Calculate results.

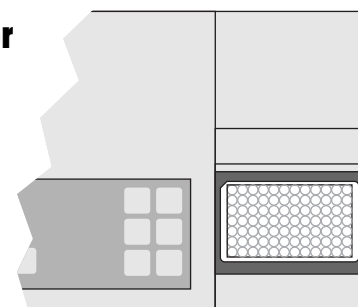

For Ordering or Technical Assistance Contact:
ABRAXIS, LLC
54 Steamwhistle Drive, Warminster, PA 18974
Phone: 215-357-3911 Fax: 215-357-5232
www.abraxiskits.com