

Importance of Metolachlor Determination

Metolachlor is one of the most widely used herbicides in agriculture throughout the world. It is a pre-emergence herbicide used on a variety of crops including corn, soybeans, peanuts and cotton. An aniline derivative and member of the chloracetanilide family of herbicides, Metolachlor was originally produced as a mixture of the S- and R-isomers (only the S-isomer is active). Modern production methods produce only the S-isomer. Metolachlor may be used alone or in combination with other herbicides. Metolachlor readily leaches into run-off and has been found in both surface and ground waters.

The Abraxis Metolachlor ELISA allows the determination of 40 samples in duplicate determination. Only a few milliliters of sample are required. The test can be performed in less than 1 hour.

Performance Data

Test sensitivity: The limit of detection for Metolachlor, calculated as 90% B/Bound, is approximately 0.058 ng/mL. The concentration of residue necessary to cause 50% inhibition (50% B/B₀) is approximately 1.6 ng/mL. Determinations closer to the middle of the calibration range of the test yield the most accurate results.

Test reproducibility: Coefficients of variation (CVs) for standards: <10%; CVs for samples: <15%.

Recoveries: Five (5) groundwater samples were spiked with various levels of Metolachlor and assayed using the Abraxis Metolachlor Plate ELISA. The following results were obtained:

Metolachlor Added (ppb)	Mean Recovery (ppb)	S.D. (ppb)	% Recovery
0.5	0.52	0.04	104
1.0	1.08	0.10	108
2.0	2.22	0.15	111
3.0	3.33	0.25	111
4.0	4.19	0.32	105
Average			108

Selectivity: This ELISA recognizes Metolachlor and related acetanilides to varying degrees:

Cross-Reactivity:	Metolachlor	100%
	Metolachlor S	100%
	Acetochlor	9%
	Butachlor	9%
	Alachlor	3%
	Metalaxyl	1%

The following compounds demonstrated no reactivity in the Abraxis Metolachlor Plate ELISA at concentrations up to 1000ppb: Aldicarb, Aldicarb Sulfate, Aldicarb Sulfone, Atrazine, Ametryn, Benomyl, Butylate, Captan, Carbaryl, Carbendazim, Carbofuran, Cyanazine, 2,4-D, 1,3-dichloropropene, Dinoseb, MCPA, Metribuzin, Pentachlorophenol, Picloram, Propazine, Simazine, Terbufos, Thiabendazole, and Thiophanate-methyl.

General Limited Warranty: Abraxis LLC warrants the products manufactured by the Company against defects and workmanship when used in accordance with the applicable instructions for a period not to extend beyond the product's printed expiration date. **Abraxis makes no other warranty, expressed or implied. There is no warranty of merchantability or fitness for a particular purpose.**

For ordering or technical assistance contact: Abraxis LLC
54 Steamwhistle Drive
Warminster, PA 18974
Tel.: (215) 357-3911
Fax: (215) 357-5232
Email: info@abraxiskits.com
WEB: www.abraxiskits.com

102909

Metolachlor ELISA, Microtiter Plate

Enzyme-Linked Immunosorbent Assay for the Determination
of Metolachlor in Contaminated Samples

Product No. 500065



1. General Description

The Metolachlor ELISA is an immunoassay for the detection of Metolachlor. This test is suitable for the quantitative and/or qualitative detection of Metolachlor in contaminated samples. Samples requiring regulatory action should be confirmed by HPLC, GC/MS, or other conventional methods.

2. Safety Instructions

The standard solutions in this test kit contain small amounts of Metolachlor. In addition, the substrate solution contains tetramethylbenzidine and the stop solution contains diluted sulfuric acid. Avoid contact of stopping solution with skin and mucous membranes. If these reagents come in contact with the skin, wash with water.

3. Storage and Stability

The Metolachlor ELISA kit should be stored in the refrigerator (4–8°C). The solutions must be allowed to reach room temperature (20–25°C) before use. Reagents may be used until the expiration date on the box.

Consult state, local and federal regulations for the proper disposal of all reagents.

4. Test Principle

The test is a direct competitive ELISA based on the recognition of Metolachlor by specific antibodies. Metolachlor, when present in a sample, and a Metolachlor-enzyme conjugate compete for the binding sites of rabbit anti-Metolachlor antibodies in solution. The Metolachlor antibodies are then bound by a second antibody (goat anti-rabbit) immobilized on the microtiter plate. After a washing step and addition of the substrate solution, a color signal is produced. The intensity of the blue color is inversely proportional to the concentration of Metolachlor present in the sample. The color reaction is stopped after a specified time and the color is evaluated using a microplate ELISA photometer. The concentrations of the samples are determined by interpolation using the standard curve constructed with each run.

5. Limitations of the Metolachlor ELISA, Possible Test Interference

Numerous organic and inorganic compounds commonly found in samples have been tested and found not to interfere with this test. However, due to the high variability of compounds that might be found in samples, test interferences caused by matrix effects cannot be completely excluded. Mistakes in handling the test can also cause errors. Possible sources for such errors can be:

Inadequate storage conditions of the test kit, incorrect pipetting sequence or inaccurate volumes of the reagents, too long or too short incubation times during the immune and/or substrate reaction, extreme temperatures during the test performance (lower than 10°C or higher than 30°C).

The Abraxis Metolachlor ELISA kit provides screening results. As with any analytical technique (GC, HPLC, etc.) samples requiring regulatory action should be confirmed by an alternative method.

A. Reagents and Materials Provided

1. Microtiter plate coated with a second antibody (goat anti-rabbit).
2. Metolachlor Standards (7) and Control (1): 0, 0.1, 0.25, 0.5, 1.0, 2.0, 5.0 ng/mL. Control at 1.5 ng/mL.
3. Antibody Solution (rabbit anti-Metolachlor), 6 mL.
4. Metolachlor-HRP Conjugate Solution, 6 mL.
5. Sample Diluent, 25 mL. Use to dilute samples.
6. Wash Solution (5X) Concentrate, 100 mL.
7. Color (Substrate) Solution (TMB), 12 mL.
8. Stop Solution, 6 mL.

B. Test Preparation

Micro-pipetting equipment and pipette tips for pipetting the standards and the samples are necessary. We recommend using a multi-channel pipette or a stepping pipette for adding the antibody, conjugate, substrate solution and stop solution in order to equalize the incubations periods of the standard solutions and the samples on the entire microtiter plate. Please use only the reagents and standards from one package lot in one test, as they have been adjusted in combination.

1. Adjust the microtiter plate and the reagents to room temperature before use.
2. Remove the number of microtiter plate strips required from the foil bag. The remaining strips are stored in the foil bag and zip-locked closed. Store the remaining kit in the refrigerator (4-8°C).
3. The standard solutions, antibody, conjugate, substrate and stop solutions are ready to use and do not require any further dilutions.
4. Dilute the Wash Buffer at a ratio of 1:5. If using the entire bottle (100 mL), add to 400 mL of deionized or distilled water.
5. The stop solution should be handled with care as it contains diluted H₂SO₄.

C. Assay Procedure

1. Add 50 µL of the **standard solutions and samples** into the wells of the test strips according to the working scheme given. We recommend using duplicates or triplicates.
2. Add 50 µL of **enzyme conjugate solution** to the individual wells successively using a multi-channel pipette or a stepping pipette.
3. Add 50 µL of **antibody solution** to the individual wells successively using a multi-channel pipette or a stepping pipette. Cover the wells with parafilm or tape and mix the contents by moving the strip holder in a circular motion on the benchtop for 30 seconds. Be careful not to spill contents.
4. Incubate the strips for 30 minutes at room temperature.
5. After incubation, remove the covering and vigorously shake the contents of these wells into a sink. Wash the strips **three times** using the 1X washing buffer solution. Use at least a volume of 250 µL of washing buffer for each well and each washing step. Remaining buffer in the wells should be removed by patting the plate dry on a stack of paper towels.
6. Add 100 µL of **color (substrate) solution** to the wells. Cover the wells with parafilm or tape and mix the contents by moving the strip holder in a circular motion on the benchtop for 30 seconds. Incubate the strips for 20 minutes at room temperature. Protect the strips from direct sunlight.
7. Add 50 µL of **stop solution** to the wells in the same sequence as for the substrate solution.
8. Read the absorbance at 450 nm using a microplate ELISA photometer within 15 minutes after the addition of the stopping solution.

D. Evaluation

The evaluation of the ELISA can be performed using commercial ELISA evaluation programs 4-Parameter (preferred) or Logit/Log. For manual evaluation, calculate the mean absorbance value for each of the standards. Calculate the %B/B₀ for each standard by dividing the mean absorbance value for each standard by the Zero Standard (Standard 0) mean absorbance. Construct a standard curve by plotting the %B/B₀ for each standard on the vertical linear (y) axis versus the corresponding Metolachlor concentration

on the horizontal logarithmic (x) axis on graph paper. %B/B₀ for samples will then yield levels in ppb of Metolachlor by interpolation using the standard curve. Samples showing lower concentrations of Metolachlor compared to Standard 1 (0.1 ng/mL) are considered as negative. Samples showing a higher concentration than Standard 5 (5.0 ng/mL) must be diluted further to obtain accurate results.

E. Additional Materials (not delivered with the test kit)

1. Micro-pipettes with disposable plastic tips (10-200 and 200-1000 µL)
2. Multi-channel pipette (10-250 µL) or stepper pipette with plastic tips (10-250 µL)
3. Microtiter plate washer (optional)
4. Microtiter plate reader (wave length 450 nm)
5. Shaker for microtiter plates (optional)
6. Timer
7. Tape or Parafilm

F. Working Scheme

The microtiter plate consists of 12 strips of 8 wells, which can be used individually for the test. The standards must be run with each test. Never use the values of standards which have been determined in a test performed previously.

Std 0-Std 6: Standards:
0; 0.1; 0.25; 0.5; 1.0; 2.0; 5.0 ppb


C: Control: 1.5 +/- 0.3 ppb

Sam1, Sam2, etc.: Samples

	1	2	3	4	5	6	7	8	9	10	11	12
A	Std 0	Std 1	Sam1									
B	Std 0	Std 1	Sam1									
C	Std 1	Std 5	Sam2									
D	Std 1	Std 5	Sam2									
E	Std 2	Std 4	rk.									
F	Std 2	Std 4	rk.									
G	Std 3	C										
H	Std 3	C										

G. Standard Curve


These values are used for demonstration purposes only; do not use these values for your determinations.

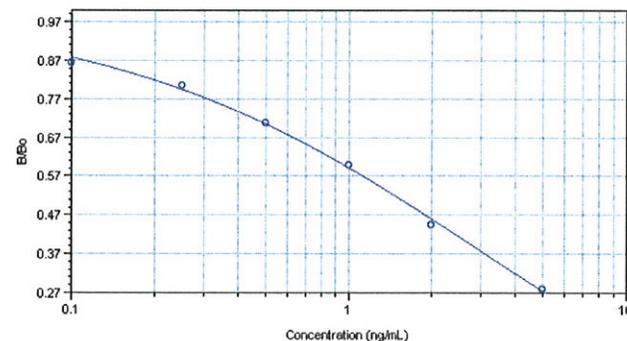

METOLACHLOR Plate, Detailed ELISA Procedure


1. Addition of Standards, Samples

Add 50 μ L of the standard solutions, control or samples into the wells of the test strips according to the working scheme given. We recommend using duplicates or triplicates.

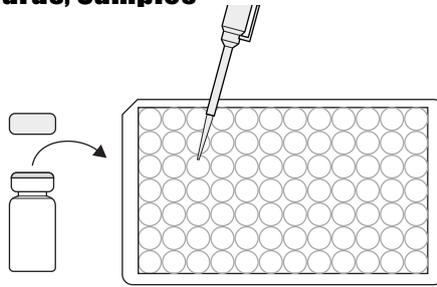


2. Addition of Enzyme Conjugate

Add 50 μ L of the Metolachlor enzyme conjugate to the individual wells successively using a multi-channel pipette or a stepping pipette.

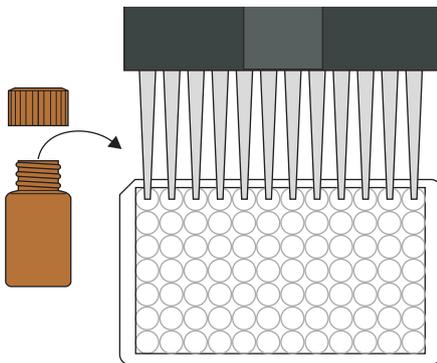


3. Addition of Antibody Solution

Add 50 μ L of the Metolachlor antibody solution to the individual wells successively using a multi-channel pipette. Cover the wells with parafilm or tape and mix the contents by moving the strip holder in a rapid circular motion on the benchtop. Be careful not to spill contents. Incubate the strips for 30 minutes at room temperature.

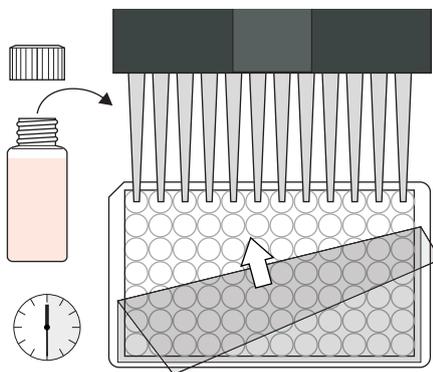


4. Washing of Plates

After incubation, remove the covering and vigorously shake the contents of the wells into a sink. Wash the strips three times with a multi-channel pipette or wash bottle using the diluted 1X washing buffer solution. Please use at least 250 μ L of washing buffer for each well and each washing step. Remaining buffer in the wells should be removed by patting the plate dry on a stack of paper towels.




5. Addition of Substrate/Color Solution

Add 100 μ L of substrate/color solution to the individual wells successively using a multi-channel pipette or a stepping pipette. Cover the wells with parafilm or tape and mix the contents by moving the strip holder in a rapid circular motion on the benchtop. Be careful not to spill contents. Incubate the strips for 20 minutes at room temperature away from direct sunlight.

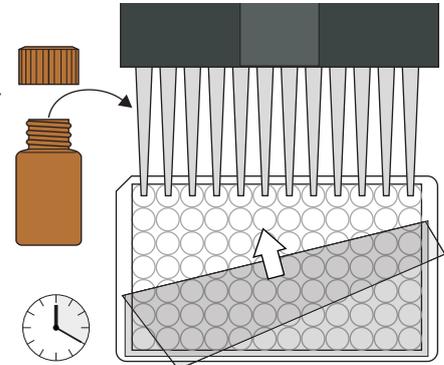


6. Addition of Stopping Solution

Add 50 μ L of stop solution to the wells, in the same sequence as for the substrate solution, using a multi-channel pipette or a stepping pipette.

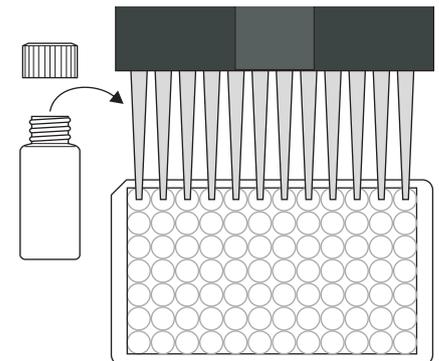

7. Measurement of Color

Read the absorbance at 450 nm using a microplate ELISA reader within 15 minutes. Calculate results.

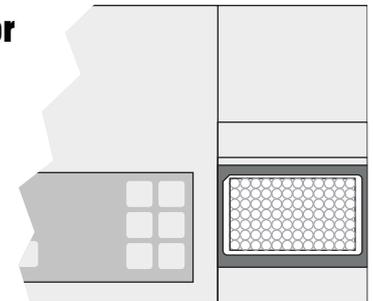


For Ordering or Technical Assistance Contact:
ABRAXIS, LLC
54 Steamwhistle Drive, Warminster, PA 18974
Phone: 215-357-3911 Fax: 215-357-5232
www.abraxiskits.com

METOLACHLOR Plate, Concise ELISA Procedure


1. Addition of Standards, Samples

Add 50 μ L of standard solutions, control or samples.

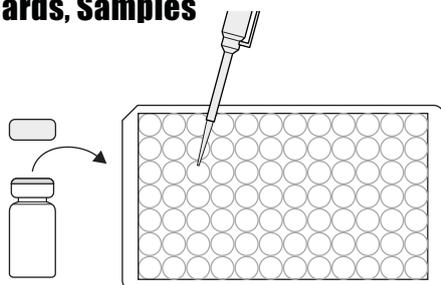


2. Addition of Enzyme Conjugate

Add 50 μ L of enzyme conjugate.

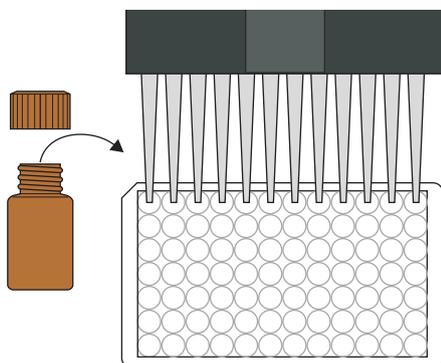


3. Addition of Antibody Solution

Add 50 μ L of the antibody solution. Cover and mix for 30 seconds by moving strip holder in a circular motion on benchtop. Incubate for 30 minutes at room temperature.

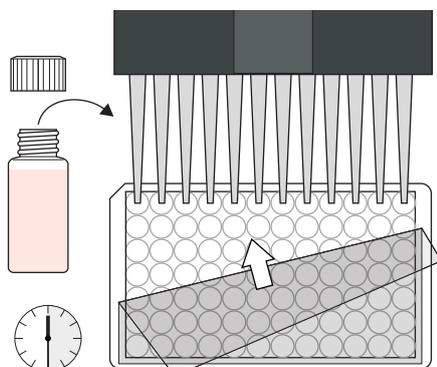


4. Washing of Plates

Wash the wells three times with 250 μ L of diluted 1X washing buffer.




5. Addition of Substrate/Color Solution

Add 100 μ L of substrate/color solution. Cover and mix for 30 seconds by moving strip holder in a circular motion on benchtop. Incubate for 20 minutes at room temperature away from direct sunlight.

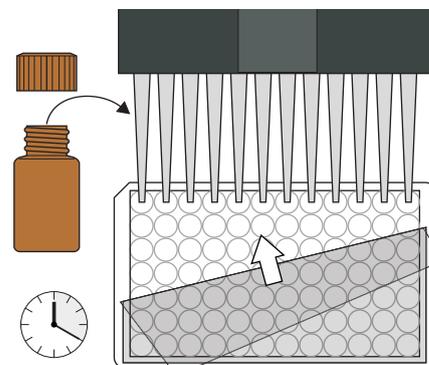


6. Addition of Stopping Solution

Add 50 μ L of stop solution.

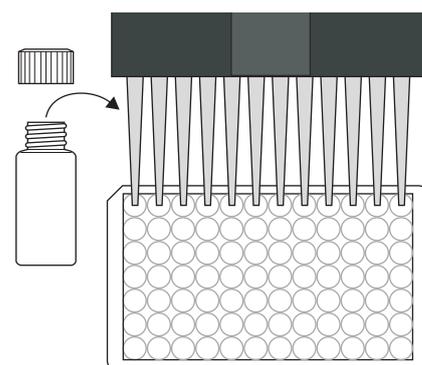

7. Measurement of Color

Measure color at 450 nm within 15 minutes. Calculate results.

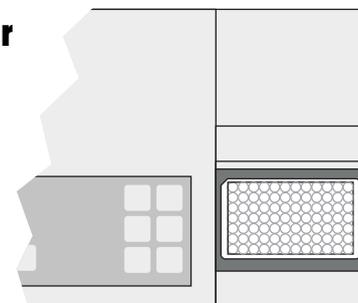

For Ordering or Technical Assistance Contact:
ABRAXIS, LLC
54 Steamwhistle Drive, Warminster, PA 18974
Phone: 215-357-3911 Fax: 215-357-5232
www.abraxiskits.com